


1 of 5

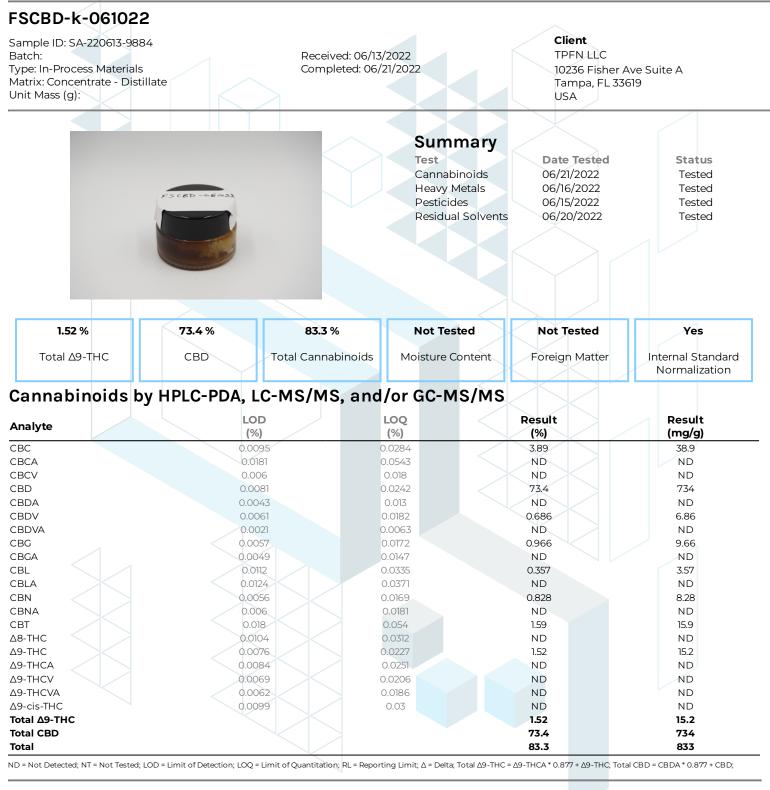

RED

Generated By: Ryan Bellone Commercial Director Date: 06/21/2022

Testéd By: Jared Burkhart Technical Manager Date: 06/21/2022



This product or substance has been tested by KCA Laboratories using validated testing methodologies and an ISO/IEC 170252017 accredited quality system. Values reported relate only to the product or substance tested. The reported result is based on a sample weight. Unless otherwise stated, results of tests performed on all quality control samples met criteria for acceptance established by KCA Laboratories. KCA Laboratories makes no claims as to the efficacy, safety or other risks associated with any detected or non-detected amounts of any substances reported herein. This Certificate of Analysis shall not be reproduced except in full, without the written approval of KCA Laboratories. KCA Laboratories to reproduce an provide measurement uncertainty upon request.



2 of 5

FSCBD-k-06102	22		
Sample ID: SA-220613-98 Batch: Type: In-Process Materia Matrix: Concentrate - Dis Unit Mass (g):	ls	Received: 06/13/2022 Completed: 06/21/2022	Client TPFN LLC 10236 Fisher Ave Suite A Tampa, FL 33619 USA
Heavy Metals k	by ICP-MS		
Analyte	LOD (ppb)	LOQ (ppb)	Result (ppb)
Arsenic	2	20	ND
Cadmium	1	20	ND
Lead	2	20	ND
Mercury	12	50	ND

ND = Not Detected; NT = Not Tested; LOD = Limit of Detection; LOQ = Limit of Quantitation; P = Pass; F = Fail; RL = Reporting Limit

Generated By: Ryan Bellone Commercial Director Date: 06/21/2022

Tested By: Nicholas Howard

estéd By: Nicholas Howarc Scientist Date: 06/16/2022



This product or substance has been tested by KCA Laboratories using validated testing methodologies and an ISO/IEC 170252017 accredited quality system. Values reported relate only to the product or substance tested. The reported result is based on a sample weight. Unless otherwise stated, results of tests performed on all quality control samples met criteria for acceptance established by KCA Laboratories. KCA Laboratories makes no claims as to the efficacy, safety or other risks associated with any detected or non-detected amounts of any substances reported herein. This Certificate of Analysis shall not be reproduced except in full, without the written approval of KCA Laboratories. KCA Laboratories can provide measurement uncertainty upon request.



3 of 5

## FSCBD-k-061022

Sample ID: SA-220613-9884 Batch: Type: In-Process Materials Matrix: Concentrate - Distillate Unit Mass (g):

Received: 06/13/2022 Completed: 06/21/2022 **Client** TPFN LLC 10236 Fisher Ave Suite A Tampa, FL 33619 USA

## Pesticides by LC-MS/MS and GC-MS/MS

Analyte	LOD (ppb)	LOQ (ppb)	Result (ppb)	Analyte	LOD (ppb)	LOQ (ppb)	Result (ppb)
Acephate	30	100	ND	Hexythiazox	30	100	ND
Acetamiprid	30	100	ND	Imazalil	30	100	ND
Aldicarb	30	100	ND	Imidacloprid	30	100	ND
Azoxystrobin	30	100	ND	Kresoxim methyl	30	100	ND
Bifenazate	30	100	ND	Malathion	30	100	ND
Bifenthrin	30	100	ND	Metalaxyl	30	100	ND
Boscalid	30	100	ND	Methiocarb	30	100	ND
Carbaryl	30	100	ND	Methomyl	30	100	ND
Carbofuran	30	100	ND	Mevinphos	30	100	ND
Chloranthraniliprole	30	100	ND	Myclobutanil	30	100	ND
Chlorfenapyr	30	100	ND	Naled	30	100	ND
Chlorpyrifos	30	100	ND	Oxamyl	30	100	ND
Clofentezine	30	100	ND	Paclobutrazol	30	100	ND
Coumaphos	30	100	ND	Permethrin	30	100	ND
Daminozide	30	100	ND	Phosmet	30	100	ND
Diazinon	30	100	ND	Piperonyl Butoxide	30	100	ND
Dichlorvos	30	100	ND	Prallethrin	30	100	ND
Dimethoate	30	100	ND	Propiconazole	30	100	ND
Dimethomorph	30	100	ND	Propoxur	30	100	ND
Ethoprophos	30	100	ND	Pyrethrins	30	100	ND
Etofenprox	30	100	ND	Spinetoram	30	100	ND
Etoxazole	30	100	ND	Spinosad	30	100	ND
Fenhexamid	30 <	100	ND	Spiromesifen	30	100	ND
Fenoxycarb	30	100	ND	Spirotetramat	30	100	ND
Fenpyroximate	30	100	ND	Spiroxamine	30	100	ND
Fipronil	30	100	ND	Tebuconazole	30	100	ND
Flonicamid	30	100	ND	Thiacloprid	30	100	ND
Fludioxonil	30 <	100	ND	Thiamethoxam	30	100	ND
		ЖГÌ		Trifloxystrobin	30	100	ND

ND = Not Detected; NT = Not Tested; LOD = Limit of Detection; LOQ = Limit of Quantitation; P = Pass; F = Fail; RL = Reporting Limit

Generated By: Ryan Bellone Commercial Director Date: 06/21/2022

Suppos Testéd By: Jared Burkhart

estéd By: Jared Burkhaı Technical Manager Date: 06/15/2022



This product or substance has been tested by KCA Laboratories using validated testing methodologies and an ISO/IEC 170252017 accredited quality system. Values reported relate only to the product or substance tested. The reported result is based on a sample weight. Unless otherwise stated, results of tests performed on all quality control samples met criteria for acceptance established by KCA Laboratories. KCA Laboratories makes no claims as to the efficacy, safety or other risks associated with any detected or non-detected amounts of any substances reported herein. This Certificate of Analysis shall not be reproduced except in full, without the written approval of KCA Laboratories. KCA Laboratories can provide measurement uncertainty upon request.



4 of 5

## FSCBD-k-061022

Sample ID: SA-220613-9884 Batch: Type: In-Process Materials Matrix: Concentrate - Distillate Unit Mass (g):

Received: 06/13/2022 Completed: 06/21/2022 **Client** TPFN LLC 10236 Fisher Ave Suite A Tampa, FL 33619 USA

# Residual Solvents by HS-GC-MS/MS

Analyte	LOD	LOQ	Result	Analyte	LOD	LOQ	Result
	(ppm)	(ppm)	(ppm)		(ppm)	(ppm)	(ppm)
Acetone	167	500	ND	Ethylene Glycol	21	62	ND
Acetonitrile	14	41	ND	Ethylene Oxide	0.5	1	ND
Benzene	0.5	1	ND	Heptane	167	500	ND
Butane	167	500	ND	n-Hexane	10	29	ND
1-Butanol	167	500	ND	Isobutane	167	500	ND
2-Butanol	167	500	ND	Isopropyl Acetate	167	500	ND
2-Butanone	167	500	ND	Isopropyl Alcohol	167	500	ND
Chloroform	2	6	ND	Isopropylbenzene	167	500	ND
Cyclohexane	129	388	ND	Methanol	100	300	ND
1,2-Dichloroethane	0.5	1	ND	2-Methylbutane	10	29	ND
1,2-Dimethoxyethane	4	10	ND	Methylene Chloride	20	60	ND
Dimethyl Sulfoxide	167	500	ND	2-Methylpentane	10	29	ND
N,N-Dimethylacetamide	37	109	ND	3-Methylpentane	10	29	ND
2,2-Dimethylbutane	10	29	ND	n-Pentane	167	500	ND
2,3-Dimethylbutane	10	29	ND	1-Pentanol	167	500	ND
N,N-Dimethylformamide	30	88	ND	n-Propane	167	500	ND
2,2-Dimethylpropane	167	500	ND	1-Propanol	167	500	ND
1,4-Dioxane	13	38	ND	Pyridine		20	ND
Ethanol	167	500	ND	Tetrahydrofuran	24	72	ND
2-Ethoxyethanol	6	16	ND	Toluene	30	89	ND
Ethyl Acetate	167	500	ND	Trichloroethylene	3	8	ND
Ethyl Ether	167	500	ND	Tetramethylene Sulfone	6	16	ND
Ethylbenzene	3	7	ND	Xylenes (o-, m-, and p-)	73	217	ND

ND = Not Detected; NT = Not Tested; LOD = Limit of Detection; LOQ = Limit of Quantitation; P = Pass; F = Fail; RL = Reporting Limit



Generated By: Ryan Bellone Commercial Director Date: 06/21/2022

Tested By: Scott Caudill Senior Scientist Date: 06/20/2022



This product or substance has been tested by KCA Laboratories using validated testing methodologies and an ISO/IEC 170252017 accredited quality system. Values reported relate only to the product or substance tested. The reported result is based on a sample weight. Unless otherwise stated, results of tests performed on all quality control samples met criteria for acceptance established by KCA Laboratories. KCA Laboratories makes no claims as to the efficacy, safety or other risks associated with any detected or non-detected amounts of any substances reported herein. This Certificate of Analysis shall not be reproduced except in full, without the written approval of KCA Laboratories. KCA Laboratories and provide measurement uncertainty upon request.



5 of 5

## FSCBD-k-061022

Sample ID: SA-220613-9884 Batch: Type: In-Process Materials Matrix: Concentrate - Distillate Unit Mass (g):

Received: 06/13/2022 Completed: 06/21/2022

#### Client

TPFN LLC 10236 Fisher Ave Suite A Tampa, FL 33619 USA

# **Reporting Limit Appendix**

Heavy Metals - Colorado CDPHE

Analyte	Limit (ppb) Ana	lyte Limit (ppb)
Arsenic	1500 Lead	500
Cadmium	500 Merce	ury 1500

#### Residual Solvents - USP 467

Analyte		Limit (ppm)	Analyte	Limit (ppm)
Acetone		5000	Ethylene Glycol	620
Acetonitrile		410	Ethylene Oxide	1
Benzene		2	Heptane	5000
Butane		5000	n-Hexane	290
1-Butanol		5000	Isobutane	5000
2-Butanol		5000	Isopropyl Acetate	5000
2-Butanone		5000	Isopropyl Alcohol	5000
Chloroform		60	Isopropylbenzene	5000
Cyclohexane		3880	Methanol	3000
1,2-Dichloroethane		5	2-Methylbutane	290
1,2-Dimethoxyethane		100	Methylene Chloride	600
Dimethyl Sulfoxide		5000	2-Methylpentane	290
N,N-Dimethylacetamic	de	1090	3-Methylpentane	290
2,2-Dimethylbutane		290	n-Pentane	5000
2,3-Dimethylbutane		290	1-Pentanol	5000
N,N-Dimethylformami	de	880	n-Propane	5000
2,2-Dimethylpropane		5000	1-Propanol	5000
1,4-Dioxane		380	Pyridine	200
Ethanol		5000	Tetrahydrofuran	720
2-Ethoxyethanol		160	Toluene	890
Ethyl Acetate		5000	Trichloroethylene	80
Ethyl Ether		5000	Tetramethylene Sulfone	160
Ethylbenzene	$\left \right $	70	Xylenes (o-, m-, and p-)	2170

# Pesticides - CA DCC

Analyte	Limit (ppb)	Analyte	Limit (ppb)	
Chloranthraniliprole	40000	Myclobutanil	9000	
Chlorfenapyr	30	Naled	500	
Chlorpyrifos	30	Oxamyl	200	
Clofentezine	500	Paclobutrazol	30	
Coumaphos	30	Permethrin	20000	
Daminozide	30	Phosmet	200	
Diazinon	200	Piperonyl Butoxide	8000	
Dichlorvos	30	Prallethrin	400	
Dimethoate	30	Propiconazole	20000	
Dimethomorph	20000	Propoxur	30	
Ethoprophos	30	Pyrethrins	1000	
Etofenprox	30	Spinetoram	3000	
Etoxazole	1500	Spinosad	3000	
Fenhexamid	10000	Spiromesifen	12000	
Fenoxycarb	30	Spirotetramat	13000	
Fenpyroximate	2000	Spiroxamine	30	
Fipronil	30	Tebuconazole	2000	
Flonicamid	2000	Thiacloprid	30	
Fludioxonil	30000	Thiamethoxam	4500	

#### Pesticides - CA DCC

Analyte	Limit (ppb)	Analyte	Limit (ppb)
Acephate	5000	Hexythiazox	2000
Acetamiprid	5000	Imazalil	30
Aldicarb	30	Imidacloprid	3000
Azoxystrobin	40000	Kresoxim methyl	1000
Bifenazate	5000	Malathion	5000
Bifenthrin	500	Metalaxyl	15000
Boscalid	10000	Methiocarb	30
Carbaryl	500	Methomyl	100
Carbofuran	30	Mevinphos	30



This product or substance has been tested by KCA Laboratories using validated testing methodologies and an ISO/IEC 170252017 accredited quality system. Values reported relate only to the product or substance tested. The reported result is based on a sample weight. Unless otherwise stated, results of tests performed on all quality control samples met criteria for acceptance established by KCA Laboratories. KCA Laboratories no claims as to the efficacy, safety or other risks associated with any detected or non-detected amounts of any substances reported herein. This Certificate of Analysis shall not be reproduced except in full, without the written approval of KCA Laboratories. KCA Laboratories to the efficacy safety or other risks associated with any detected or non-detected amounts of any substances reported herein. This Certificate of Analysis shall not be reproduced except in full, without the written approval of KCA Laboratories. KCA Laboratories can provide measurement uncertainty upon request.